


## ColoQuick Pasteur

# HOW TO REPLACE CONTROL UNIT



- 1) Disconnect electrical connectors
- 2) Unscrew; x8 screws (hold on to the nuts using pliers)

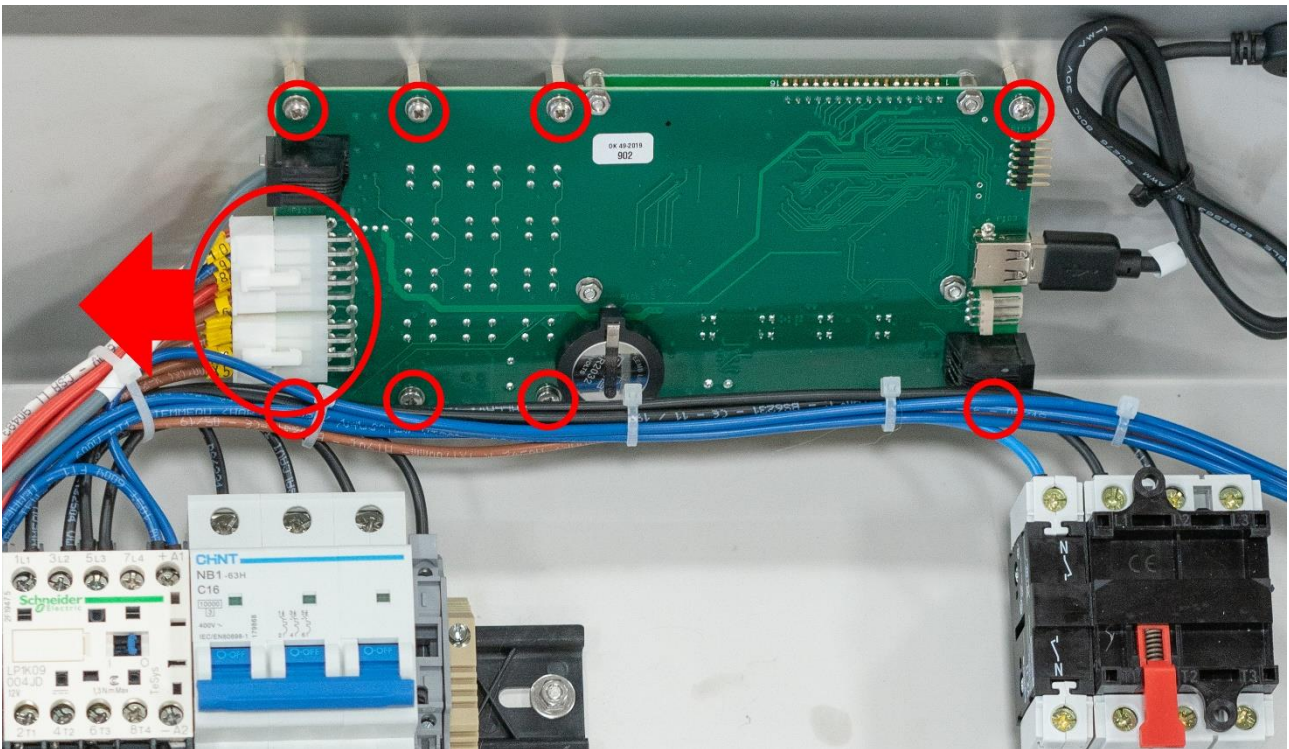